

**THIS PAGE IS INSERTED BY OIPE SCANNING  
AND IS NOT PART OF THE OFFICIAL RECORD**

**Best Available Images**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

**BLACK BORDERS** ✓

**TEXT CUT OFF AT TOP, BOTTOM OR SIDES**

**FADED TEXT**

**BLURRY OR ILLEGIBLE TEXT**

**SKEWED/SLANTED IMAGES**


**COLORED PHOTOS HAVE BEEN RENDERED INTO BLACK AND WHITE**

**VERY DARK BLACK AND WHITE PHOTOS**

**UNDECIPHERABLE GRAY SCALE DOCUMENTS**

**IMAGES ARE THE BEST AVAILABLE  
COPY. AS RESCANNING *WILL NOT*  
CORRECT IMAGES, PLEASE DO NOT  
REPORT THE IMAGES TO THE  
PROBLEM IMAGE BOX.**





Europäisches Patentamt  
European Patent Office  
Office européen des brevets



(11) EP 0 850 651 A2

(12) EUROPEAN PATENT APPLICATION

(43) Date of publication:  
01.07.1998 Bulletin 1998/27

(51) Int. Cl.<sup>6</sup>: A61L 27/00, A61L 31/00

(21) Application number: 97203933.3

(22) Date of filing: 15.12.1997

(84) Designated Contracting States:  
AT BE CH DE DK ES FI FR GB GR IE IT LI LU MC  
NL PT SE  
Designated Extension States:  
AL LT LV MK RO SI

(72) Inventor: Ding, Ni  
Plymouth, Minnesota 55446 (US)

(74) Representative: Jansen, Götz  
Schneider (Europe) AG,  
Ackerstrasse 6  
8180 Bülach (CH)

(30) Priority: 20.12.1996 US 33443 P

(71) Applicant: SCHNEIDER (USA) INC.  
Plymouth, Minnesota 55442 (US)

(54) Method of applying drug-release coatings

(57) The invention is directed to a method of applying drug-release coatings whereby a polymer can be dissolved in a first solvent (solvent A) to form a polymer system and a drug can be dissolved or suspended in a second solvent (solvent B) to form a drug system. The coating or layer of coating so formed comprises a substantially uniform combination of the drug and polymer. Solvent B can be the same as or different than solvent A. The coating can be applied on a stent body by separately spraying or dipping the polymer system and the drug system onto the devices. The coating can be accomplished by either applying the polymer and drug systems sequentially or simultaneously. In certain embodiments, a drug can be suspended in solvent B. In some cases, three or more systems can be utilized. For instance, a third system containing pure solvent A or B can smooth the coating surface, if the solvent of the third spraying system is compatible with the polymer matrix.

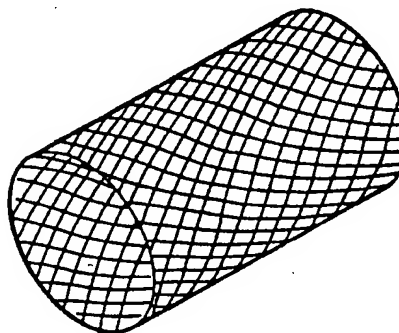


FIG. 10

EP 0 850 651 A2

## Description

This application claims priority to U.S. Provisional Application Serial No. 60/033,443 filed December 20, 1996.

## Field of the Invention

This invention relates generally to drug-releasing coatings for medical devices which are inserted or implanted into the body. More particularly, the invention is directed to a method for applying drug-releasing coatings to medical devices in which a polymer is dissolved in a first solvent (solvent A) to form a polymer system and a drug is dissolved in a second solvent (solvent B) to form a drug system.

## Background of the Invention

In prior art methods, a composition comprising a mix of a drug and a polymer in a solvent is applied to the device to form a substantially uniform layer of drug and polymer; *i.e.* a layer in which the drug is dispersed in the polymer in a substantially uniform manner. Depending upon the types of polymers and drugs employed, finding a common solvent for these two constituents can be problematic. Where a common solvent for the drug and polymer is not available, attempts have been made to micronize the drug into small particles so that it can be suspended in the polymer solution. However, micronization can be time consuming, and may result in a loss of desired therapeutic properties of the drug. Therefore, a method of more easily putting both the drug and polymer into solution to obtain a drug releasing coating for medical devices is needed. Also needed is a method of applying a drug/polymer coating without having to combine the drug and polymer in a common solution or suspension.

## Summary of the Invention

The methods disclosed herein apply generally to implantable prostheses, especially expandable prostheses such as balloon expandable stents and self-expanding stents. Stents coated according to this invention may be, for instance, plastically deformable or self-expanding. In certain embodiments, the methods avoid the necessity of micronizing a drug before it is applied to a stent. In other embodiments, drug particulates can be utilized. The present invention can also be used where there is no common compatible solvent for both the polymer and the drug.

Broadly, the invention relates to a method of applying drug-release coatings containing a drug and a polymer, in which the drug is distributed in the polymer in a substantially uniform manner. A polymer can be dissolved in a first solvent (solvent A) to form a polymer system substantially free of biologically active materials

(*e.g.*, less than about 1% by weight of the polymer) and a drug can be dissolved in a second solvent (solvent B) to form a drug system substantially free of polymers (*e.g.*, less than about 1% by weight of the drug). Solvent B can be the same as or different than solvent A. Different solvents are generally used when the drug has very low solubility in the polymer solution and no common solvent would be found for both the drug and polymer. By applying the polymer system and drug system separately to the surface of the medical device, the method forms a composite of the polymer and drug, *i.e.*, a distribution of the drug throughout a network of polymer. Such composite may be substantially homogenous. The method of the present invention avoids the need for micronizing the drug prior to mixing it with the polymer to form the composite of drug and polymer. Although the method provides a coating or a layer of a coating which comprises a composite of the drug and polymer, it avoids the need for mixing the drug and polymer in one solution before applying the coating to the device.

A coating can be applied on a device, particularly a stent, by separately spraying the polymer system and the drug system. Methods of coating stents are disclosed in U.S. patent application serial nos. 08/424,884; 08/526,273; and 08/663,490. These documents are incorporated herein by reference in their entireties for all purposes. The coatings of the invention can be accomplished by either spraying the polymer and drug systems sequentially or simultaneously, as further described below.

Instead of applying the coating by spraying, the coating can also be placed onto the medical device by dipping. This latter method of applying the coating is especially useful for devices which are not conducive to being spray coated. Such devices include without limitation the inner lumen of a stent graft. Also, the coating may be applied by using a combination of spraying and dipping.

Depending upon the coating thickness desired, multi-step coatings may be applied. Depending upon the solvent volatility, a waiting period may be required during the spraying or dipping process, or heat may be applied through a heat gun, a heat lamp or a heat chamber to facilitate the evaporation of the solvent(s).

In certain embodiments, it is not necessary for a drug to be dissolved in solvent B. Fine particles can be mixed, preferably suspended, in the solvent, and the coating can be applied as described herein. In some cases, three or more systems can be utilized. For instance, a third spraying or dipping system containing pure solvent A or B can smooth the coating surface, if the solvent of the third system is compatible with the polymer matrix, or a third spraying or dipping system containing a second elutable agent such as a drug. Polyethylene glycol, sugar, salt in solvent (which can be same or different than solvents A and B), can be applied to the stent. The resulting drug release profile, where two or more drugs are applied, can result in the different

drugs being released simultaneously or sequentially.

A suitable sequence according to this invention could be one application of a polymer solution, one application of a drug solution and one application of pure solvent. Alternatively, the sequence could be one application by spraying or dipping of polymer solution, one application of solvent and one application of a drug solution or suspension. Alternatively, the sequence could be three parallel spraying systems. The number of cycles in each operation could be half, one, two or more. It is appreciated that those skilled in the art will find numerous combinations of coating orders and sequences for dual or multiple coating systems without departing from the inventive concept. The coating system can be hand-operated or automated to achieve different combinations.

### Brief Description of the Drawings

FIGURE 1 is a photograph showing the results of the Comparative Example;

FIGURE 2 is a photograph showing the results of Example 1;

FIGURE 3 is a photograph showing the results of Example 2;

FIGURES 4 and 5 are scanning electron microscope photographs showing the results of the Comparative Example in an unstressed state and a post-stressed state, respectively;

FIGURES 6 and 7 are scanning electron microscope photographs showing the results of Example 1 in an unstressed state and a post-stressed state, respectively;

FIGURES 8 and 9 are scanning electron microscope photographs showing the results of Example 2 in an unstressed state and a post-stressed state, respectively;

FIGURE 10 shows a stent prior to coating;

FIGURES 11 and 12 sequentially illustrate an embodiment of the present invention;

FIGURES 13 and 14 sequentially illustrate an alternative embodiment of the present invention;

FIGURE 15 graphically compares elution rates for the Comparative Example, Example 1 and Example 2; and

FIGURE 16 is a graphical comparison of the elution rates of Examples 4a, 4b, 5 and 6.

### Detailed Description of the Invention

Polymers suitable for the present invention will preferably be hydrophobic biostable elastomeric materials which do not degrade and which minimize tissue rejection. Furthermore, the materials are preferably ones which will undergo encapsulation by tissue adjacent to the stent implantation site. Polymers suitable for such coatings include silicones (e.g., polysiloxanes and substituted polysiloxanes), polyurethanes (including poly-

carbonate urethanes), thermoplastic elastomers in general, ethylene vinyl acetate copolymers, polyolefin elastomers, EPDM rubbers and polyamide elastomers. The above-referenced materials are considered hydrophobic with respect to the contemplated environment of the invention.

Non-limiting examples of other polymers which are suitable for use in the present invention include bioabsorbable polymers such as polylactic acid, polyglycolic acid, polycaprolactone, polylactic acid - polyethylene oxide copolymers, cellulose, and the like. Other non-limiting examples of polymers that are suitable for use in the present invention also include biostable plastic materials such as acrylic polymers and its derivatives, nylon, and polyesters.

Non-limiting examples of drugs suitable for use in the present invention include antithrombotics, anticoagulants, antiplatelet agents, thrombolytics, antiproliferatives, anti-inflammatories, agents that inhibit hyperplasia and in particular restenosis, smooth muscle cell inhibitors, antibiotics, growth factors, growth factor inhibitors, cell adhesion inhibitors, cell adhesion promoters and drugs that may enhance the formation of healthy neointimal tissue, including endothelial cell regeneration. The positive action may come from inhibiting particular cells (e.g., smooth muscle cells) or tissue formation (e.g., fibromuscular tissue) while encouraging different cell migration (e.g., endothelium) and tissue formation (neointimal tissue).

The drug used in the invention may or may not be micronized. When the drug is not micronized, the particle size of the drug can be greater than about 10  $\mu\text{m}$ . When the drug is micronized, the drug particle size is preferably 5-12  $\mu\text{m}$  and more preferably about 5  $\mu\text{m}$ .

The devices suitable for the invention include without limitation a variety of medical devices such as catheters, shunts, stents (e.g. self expandable or balloon expandable vascular or non-vascular stents), heart valves, grafts, and artificial organs or prostheses. The devices may have polymeric, metallic or ceramic surfaces.

The preferred materials for fabricating stents, particularly braided stents, such as that shown in FIGURE 10, include metals such as stainless steel, tantalum, titanium alloys including nitinol (a nickel titanium, thermomemorial alloy material), DFT materials such as shown in U.S. 5,630,840 and certain cobalt alloys including cobalt-chromium-nickel alloys such as Elgiloy<sup>®</sup> and Phynox<sup>®</sup>. Bioabsorbable materials may also be used to form the stent structure, such as polylactic acid. Further details concerning the fabrication and details of other aspects of the stents themselves are found in U.S. Patent Nos. 4,655,771 and 4,954,126 to Wallsten and 5,061,275 to Wallsten *et al.* which are incorporated herein by reference in their entireties.

Solvents which can be used in the present invention will preferably be compatible with the polymer or drug with which they are mixed. For instance, the polymer will

preferably be fully dissolvable in the solvent with which it is mixed, and the drug will preferably be fully dissolvable in the solvent with which it is mixed. However, it is contemplated that certain embodiments of the present invention will include particulate drugs, such as heparin, mixed in solvent. Where drugs are in particulate form, the drug will preferably be suspended in the solvent. Non-limiting examples of solvents that can be used according to this invention include tetrahydrofuran, methanol, methyl ethyl ketone, chloroform, methylene chloride, acetonitrile, and water.

The following examples describe embodiments of the invention in which the coatings were applied to the medical devices by spray coating (Comparative Example and Examples 1-3) or by dip coating (Examples 4-6).

#### Comparative Example

A silicone-xylene mixture (~34% solid weight from Applied Silicone Corporation) was weighed, and the solid silicone content was calculated. A ratio of  $W_{dex}/W_{silicone\ solid} = 0.1$  was used in the preparation. Here "dex" or "DEX" refers to dexamethasone (Upjohn, Dexamethasone USP, CAS # 50-02-2). The volume amount of tetrahydrofuran (THF) (HPLC grade, Aldrich or EM Science) used was determined by multiplication of 20 with the weight of the solid silicone. DEX was first dissolved in THF and then transferred to a silicone-xylene mixture. A crosslinker agent was added and the solution was mixed well. A braided stent was coated by spraying multiple cycles of the homogeneous solution so prepared on the stent in an expanded state. The coated stent was then moved to a convection oven and cured at 150°C for 45 minutes. It was then treated with argon gas plasma according to the procedure described in co-pending application Serial No.08/841,747. The results are shown in FIGURES 1, 4 and 5. FIGURES 1 and 4 are photographs of the coating in an unstressed state, i.e., before the stent was expanded or contracted. FIGURE 5 is a photograph of the coating after the coated stent was mechanically stressed, i.e., following contraction and expansion of the stent.

#### Example 1

A 5% (w/w) solution of silicone solid in THF was prepared by adding the required THF and crosslinker agent into the silicone mixture. A separate 0.5% (w/w) solution of DEX in THF was prepared by adding THF into a beaker containing DEX. The ratio of  $W_{dex}/W_{silicone\ solid}$  was 0.1. A badger 150-4 spray system was used with two reservoirs filled with two different solutions. The coating of the stent in an expanded state was accomplished by spraying one cycle of silicone solution, waiting for a short period of time (about 30 seconds), and spraying one cycle of DEX solution, waiting for a short period of time (about 30 seconds), and then repeating

the spraying sequence. The very last spray cycle was silicone solution. For a coating thickness of 30 micron, about 30 cycles each were applied. The number of spray cycles used depended on the solution viscosity, the droplet size and the flow rate. The coated stent was then moved to a convection oven and cured at 150°C for 45 minutes. It was then argon gas plasma treated. The results are shown in FIGURES 2, 6, and 7. FIGURES 2 and 6 are photographs of the coating in an unstressed state. FIGURE 7 is a photograph of the coating after the coated stent was mechanically stressed.

#### Example 2

The process used to prepare this example was similar to the process utilized in Example 1 except that DEX was dissolved in methanol, which is a poor solvent for silicone. The ratio of  $W_{dex}/W_{silicone\ solid}$  was maintained at 0.1 in the preparation. The results are shown in FIGURES 3, 8, and 9. FIGURES 3 and 8 are photographs of the coating in an unstressed state. FIGURE 9 is a photograph of the coating after the coated stent was mechanically stressed, i.e., expanded and contracted.

#### Example 3

The coated stents prepared in the Comparative Example, Example 1 and Example 2 were cut into 2 cm segments and put into 100 ml of polyethylene glycol (MW=400, Aldrich) and water mixture (40/60, v/v). The solution was changed frequently when sampling the solution. The DEX concentration was analyzed by using a Shimadzu high performance liquid chromatography instrument, operated with a UV detector at the wavelength of 254 nm. A C-8 column was used in the analysis. Table 1 and FIGURE 15 show the DEX release data over one month for the coated stents. All three preparations in the Comparative Example, Example 1 and Example 2 prolonged the drug release and had similar release profiles.

Table 1

Release Rate Data ( $\mu\text{g}/\text{cm}^2/\text{hr}$ )			
Time (days)	Comp. Ex.	Ex. 1	Ex. 2
0.08	6.25	27.46	14.88
1.73	0.66	3.32	0.83
3.77	0.38	1.08	0.36
4.75	0.38	0.91	0.33
11.81	0.24	0.44	0.21
14.08	0.24	0.34	0.22
16.94	0.23	0.27	0.20
19.08	0.22	0.28	0.22

Table 1 (continued)

Release Rate Data ( $\mu\text{g}/\text{cm}^2/\text{hr}$ )			
Time (days)	Comp. Ex.	Ex. 1	Ex. 2
21.08	0.21	0.19	0.18
26.08	0.15	0.17	0.14
28.00	0.11	0.10	0.12
32.06	0.17	0.16	0.15

An embodiment of the present invention involving spray coating is sequentially illustrated in Figures 11 and 12. The drug-release coating apparatus 2 has a stent rotating element 4 and a spraying element 6.

A stent 8 is mounted on the stent rotating element 4 by clamping it at both ends to supporting rod elements 24', 24'', which are typically alligator clamps. Preferably, stent 8 will be clamped in a position which is at least partially expanded or fully expanded such that its interior remains empty allowing spray coating to adhere to both the exterior and the interior surface of stent 8. Rod elements 24', 24'' do not traverse the interior of stent 8. Motor 10 rotates the rod elements 24', 24'' thereby rotating stent 8. Supporting rod 12 supports the stent rotating element 4.

Spraying element 6 has a structural support 14 on which a first spray canister 16 and a second spray canister 18 are mounted. First spray canister 16 is fluidly connected to first spray dispenser 20 and second spray canister 18 is fluidly connected to second spray dispenser 22. Gas supply means 26, 28 are connected to the spraying devices to provide gaseous means to propel the polymer and drug solutions.

The first and second spray canisters 16, 18 can be mounted on structural support 14 on a track (not shown) to enable longitudinal movement back and forth. In a simplified case, a hand can act as a support 14. In this embodiment, canisters 16, 18 are fixed at a predetermined distance from one another, so that they move to and from equidistant from one another. The hollow arrow in FIGURE 11 shows canisters 16, 18 prior to leftward movement. Spray will begin once spray dispensers 20, 22 oppose the stent 8. The solid arrow in FIGURE 12 shows canisters 16, 18 beginning their course back to the right, again beginning to spray once dispensers 20, 22 oppose the stent. This sequence can be repeated multiple times, as desired.

In this embodiment, first spray canister 16 can hold polymer in solvent and be free of drug, while second spray canister 18 can hold drug in solvent and be free of polymer, or *vice versa*.

FIGURES 13 and 14 sequentially illustrate a different embodiment of the present invention. The reference numerals in this embodiment have the same meaning as those in the previous embodiment shown in FIGURES 11 and 12.

The first and second spray canisters 16, 18 can be

mounted on structural support 14 on two tracks (not shown) to enable longitudinal movement back and forth. In this embodiment, canisters 16, 18 can move to and from independent from one another. In FIGURE 13, the solid arrow shows the first canister 16 moving to the left and spraying the stent, while the hollow arrow indicates second canister 18 in a stationary position with the potential to move to the left. First canister 16 continues to the left and then stops beyond the stent and assumes a stationary position (not shown). Then, as shown in FIGURE 14, the second canister 18 moves to the left to spray the stent and then rests to the left of the stent. Thereafter, the first canister 16 can move to the right, later followed by the second canister 18, and the process can be repeated as desired.

Other processes according to this invention can include the first canister 16 going to and from while the second canister 18 is at rest beyond the stent, followed by the second canister going to and from while the first canister 16 is at rest beyond the stent. Other non-limiting variations include having canisters 16 and 18 move simultaneously but spaced apart from one another, or having canisters 16 and 18 criss-cross while spraying.

In addition to spray coating, the coatings of this invention can be applied by dipping the medical device in 1) a polymer dissolved in a first solvent and 2) a drug dissolved in a second solvent. The device can be repeatedly dipped into the polymer solution and drug solution until a coating of the desired thickness is achieved. In general, the polymer will shrink and swell, and the drug will recrystallize or redistribute in the subsequent dipping steps depending upon the relative solvability of the solvents to the polymer and drug. In order to ensure uniformity of the coating on the device, certain steps can be taken. These steps include, without limitation: choosing a solvent with a low viscosity index, choosing a polymer above its entanglement molecular weight such that the inner polymer layer(s) will swell but will not be easily dissolved, blow drying the coating after each dipping, horizontally coating the device, rotating the device during drying and using short coating times.

The following examples illustrate embodiments of the invention which were prepared by dipping.

#### Example 4

15 grams of a silicone dispersion from Applied Silicone Corp. (#40000), containing 35% solids, was weighed. 0.52 grams of dexamethasone (DEX) (Upjohn, Lot #719kT) was dissolved in 15 mL of tetrahydrofuran (THF). The drug solution was added to the silicone dispersion and stirred until a homogeneous solution was formed.

A stent graft (Example 4a) was dipped into the solution and air dried in its horizontal position. The coating weight for this sample was 10.8 mg/cm<sup>2</sup>. Due to gravity, the coating became uneven. To obtain a more uniform coating, a second stent graft (Example 4b), after being

dipped into the solution, was rotated horizontally as it air dried. The coating weight for this sample was 13.5 mg/cm<sup>2</sup>. After sitting at room temperature for about 1.5 hours, the coated samples were oven cured at 150°C for 1 hour.

The grafts were cut into 2 cm pieces and their release rates were studied by immersing the pieces in a 25/75 v/v aqueous solution of polyethylene glycol (PEG) (MW=400 from J.T. Baker). The solutions were periodically sampled and replaced with fresh solution. The amount of DEX released was quantified by a Shimadzu High Performance Liquid Chromatography (HPLC), using a C8 column (Phase Separation Ltd) with a mobile phase of acetonitrile/H<sub>2</sub>O (1:1 v/v), a flow rate of 1 ml/min and a UV detector at a wavelength of 254 nm. The release rates for these two samples are presented in Table 2. The data shows that the coated samples can provide prolonged drug release (see FIGURE 16).

Table 2

Release Rate Data (μg/cm <sup>2</sup> /hr)				
Time (days)	Ex. 4a	Ex. 4b	Ex. 5	Ex. 6
0.0	75.26	61.51	23.66	63.96
0.8	14.54	16.80	6.68	22.14
3.1	5.75	6.55	3.71	4.76
5.8	3.46	3.97	2.31	2.19
8.1	2.02	2.65	1.61	1.27
10.1	1.64	2.22	1.27	0.85
12.9	1.48	2.02	1.34	1.41
16.1	1.48	1.94	1.25	1.59
19.8	1.30	1.81	1.12	0.71
22.8	1.05	1.45	0.96	0.57
27.8	0.89	1.29	0.83	0.46
30.8	0.81	1.16	0.72	0.47
37.9	0.70	1.05	0.65	0.33

#### Example 5

A silicone dispersion containing 4% silicone in THF was prepared. Also prepared was a 10% solution of DEX in THF. A stent graft was dipped into the silicone solution first and dried while being rotated for at least 1 minute. The stent was then dipped into the DEX/THF solution and rotated for at least 1 minute to dry the stent. This sequence of dipping and drying was repeated for about 20 times. The last dip was in the silicone solution. After sitting at room temperature for about 1.5 hours, the coated samples were oven cured at 150°C for 1 hour.

Like the stents in Example 4a and 4b, this sample was also cut into 2 cm pieces and the release rate was

studied according to the procedure used in Examples 4a and 4b. The release rate for Example 5 is presented in Table 2 and FIGURE 16. The data shows that the coated samples can provide prolonged drug release.

#### Example 6

The silicone dispersion of Example 5 was prepared. Also prepared was a 10% solution of DEX in methanol (MeOH), which is a poor solvent for silicone and hence incompatible to silicone. A stent graft was coated according to the method used to prepare Example 5. This sample was cut into 2 cm pieces and the release rate was studied according to the procedure used in Examples 4a and 4b. The release rate for Example 6 is presented in Table 2. The data shows that the coated samples can provide prolonged drug release although this sample exhibited a faster initial drug elution rate than Examples 4a, 4b and 5 (see FIGURE 16).

The description contained herein is for purposes of illustration and not for purposes of limitation. Changes and modifications may be made to the embodiments of the description and still be within the scope of the invention. Furthermore, obvious changes, modifications or variations will occur to those skilled in the art.

#### Claims

1. A method of making a medical device having at least a portion for insertion or implantation into the body of a patient, wherein the portion has a surface which is adapted for exposure to body tissue of the patient and wherein at least a part of the surface is covered with a coating, to release at least one biologically active material therefrom, the method comprising:

- applying a polymer system substantially free of a biologically active material comprising a polymer and a first solvent to the surface, and
- applying a drug system substantially free of a polymer comprising a biologically active material and a second solvent to the surface; wherein said method forms a composite of the polymer and the biologically active material.

2. The method of claim 1 wherein the composite is substantially homogeneous.

3. The method of claim 1 wherein steps (a) and (b) are repeated.

4. The method of claim 1 wherein the medical device is a stent.

5. The method of claim 1 wherein the stent is a self-expanding stent.



6. The method of claim 1 wherein the first solvent and second solvent are the same.
7. The method of claim 1 wherein the first solvent and second solvent are different. 5
8. The method of claim 1 wherein the polymer is a hydrophobic biostable elastomer.
9. The method of claim 1 wherein the elastomer is selected from the group consisting of silicones, polyurethanes, thermoplastic elastomers, ethylene vinyl acetate copolymers, polyolefin elastomers, EPDM rubbers and polyamide elastomers. 10
10. The method of claim 1 wherein the biologically active material is selected from the group consisting of antithrombotics, anticoagulants, antiplatelet agents, thrombolytics, antiproliferatives, anti-inflammatories, agents that inhibit hyperplasia, smooth muscle cell inhibitors, antibiotics, growth factors, growth factor inhibitors, cell adhesion inhibitors, cell adhesion promoters and drugs that may enhance the formation of healthy neointimal tissue. 15
11. The method of claim 1 wherein the polymer system or drug system is applied by spray coating. 20
12. The method of claim 1 wherein the polymer system or drug system is applied by dipping. 25
13. The method of claim 1 wherein the polymer system and the drug system are applied simultaneously to the surface. 30
14. The method of claim 1 wherein the polymer system and the drug system are applied sequentially to the surface. 35
15. The method of claim 1 which further comprises partially evaporating the first solvent prior to applying the drug system. 40
16. The method of claim 1 wherein the biologically active material is dissolved in the second solvent. 45
17. The method of claim 1 wherein the biologically active material is suspended in the second solvent.
18. The method of claim 1 which further comprises applying a solvent system to the surface. 50
19. The method of claim 1 which further comprises applying a second drug system substantially free of a polymer comprising a second biologically active material to the surface. 55
20. An apparatus 2 for covering at least part of a surface of a medical device 8 with a coating, said apparatus 2 comprising:
  - a) a mounting element 4 comprising at least one support element 24 for mounting the device 8 to the apparatus 2; and
  - b) a spray element 6 aligned with said mounting element 4 in a manner which allows the surface of the device 8 to be sprayed, said spray element 6 comprising
    - i) a structural support 14 and
    - ii) first and second spray canisters 16, 18 movably mounted on said structural support 14, wherein said first canister 16 is fluidly connected to a first spray dispenser 20 and said second canister 18 is fluidly connected to a second spray dispenser 22.
21. The apparatus 2 of claim 20 wherein gas supply means 26, 28 are connected to said first and second spray dispensers 20, 22.
22. The apparatus 2 of claim 20 wherein said first and second canisters 16, 18 are fixed at a predetermined distance from each other.
23. The apparatus 2 of claim 20 wherein said first and second canisters 16, 18 are capable of movement independent of each other.
24. The apparatus 2 of claim 20 wherein said first and second canisters 16, 18 are movably mounted on said structural support 14 in a manner which permits said canisters 16, 18 to move past one another.
25. The apparatus 2 of claim 20 which further comprises a motor 10 for rotating said support element 24.

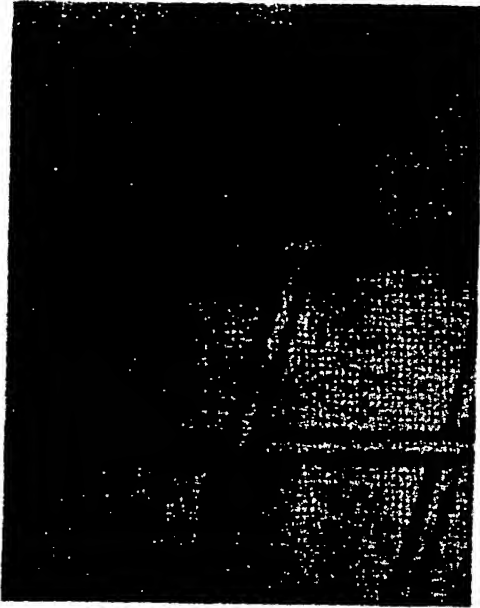


FIG. 1

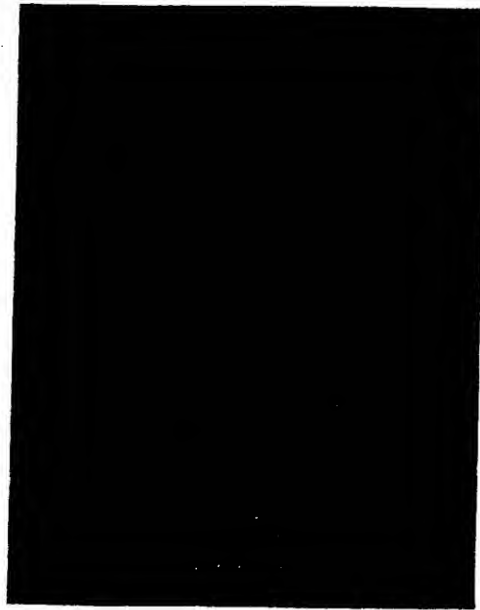


FIG. 2

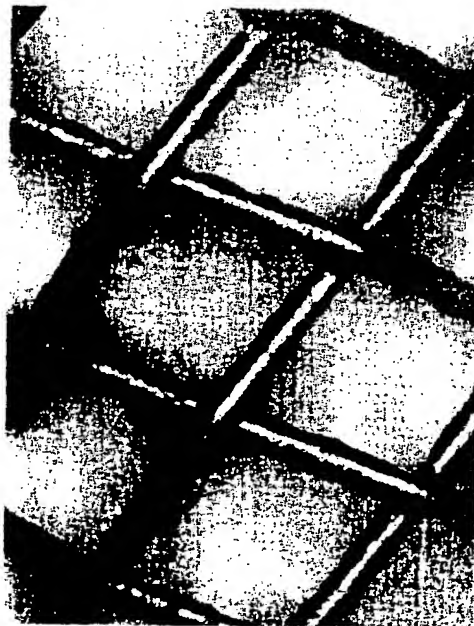


FIG. 3



FIG.4



FIG.5



FIG.6



FIG.7

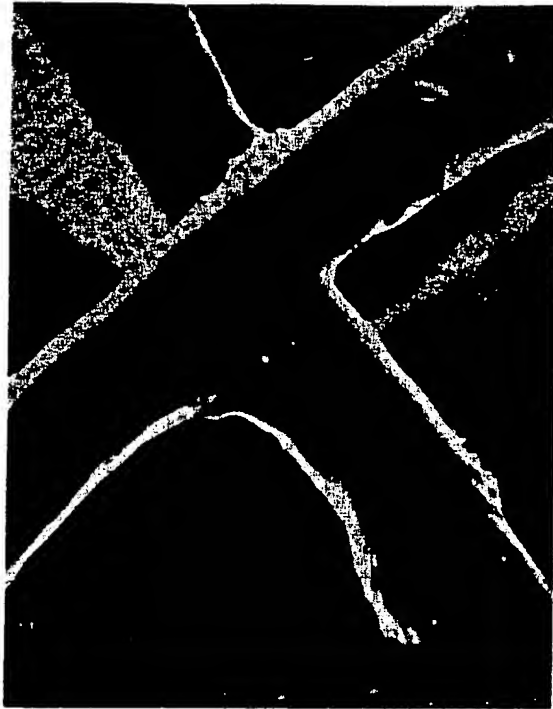


FIG. 8



FIG. 9

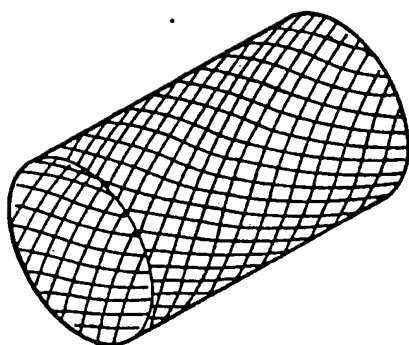
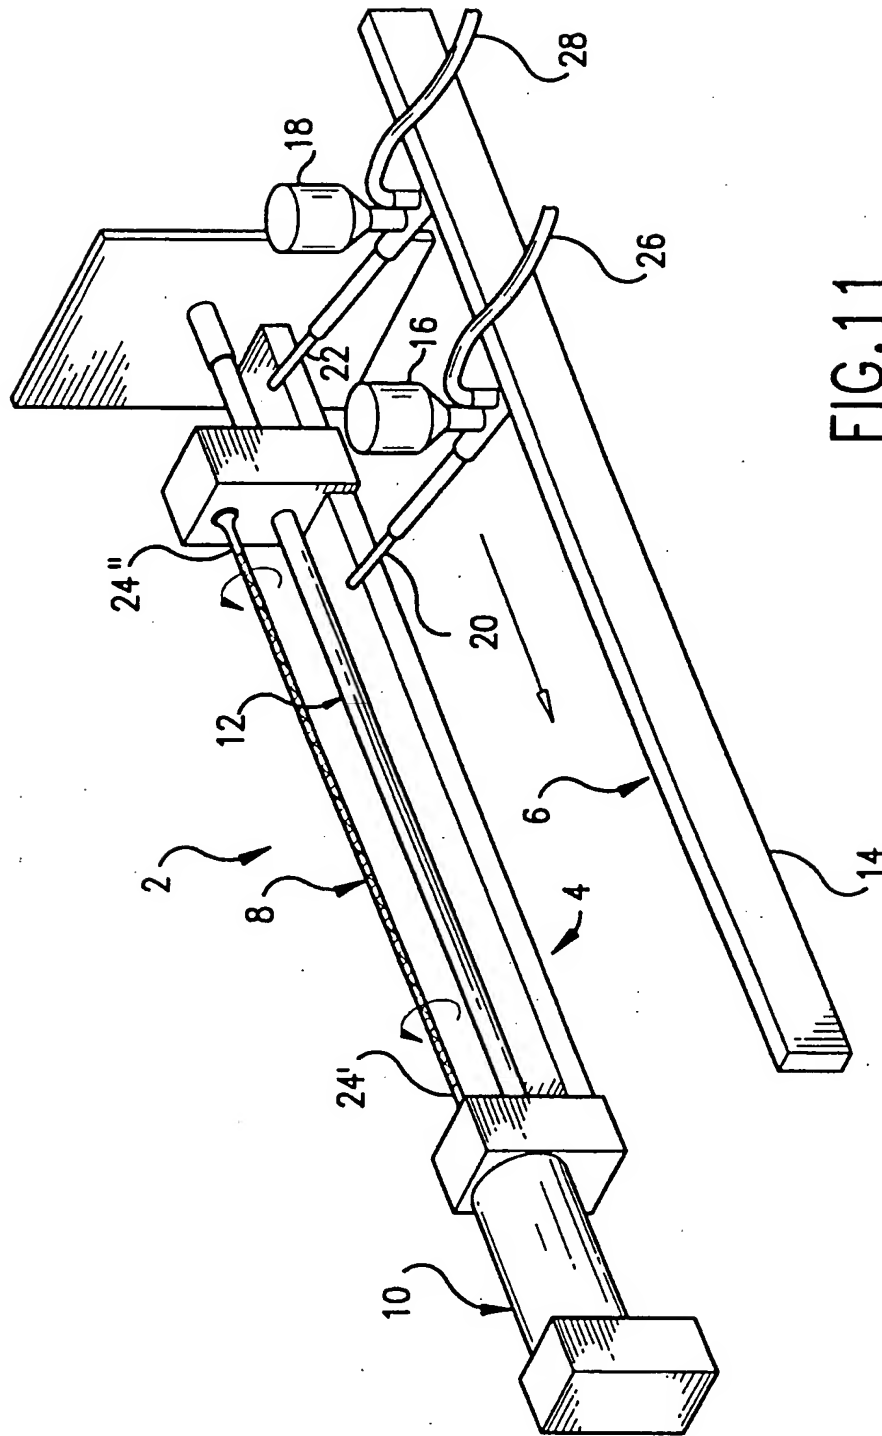


FIG. 10



**FIG. 11**

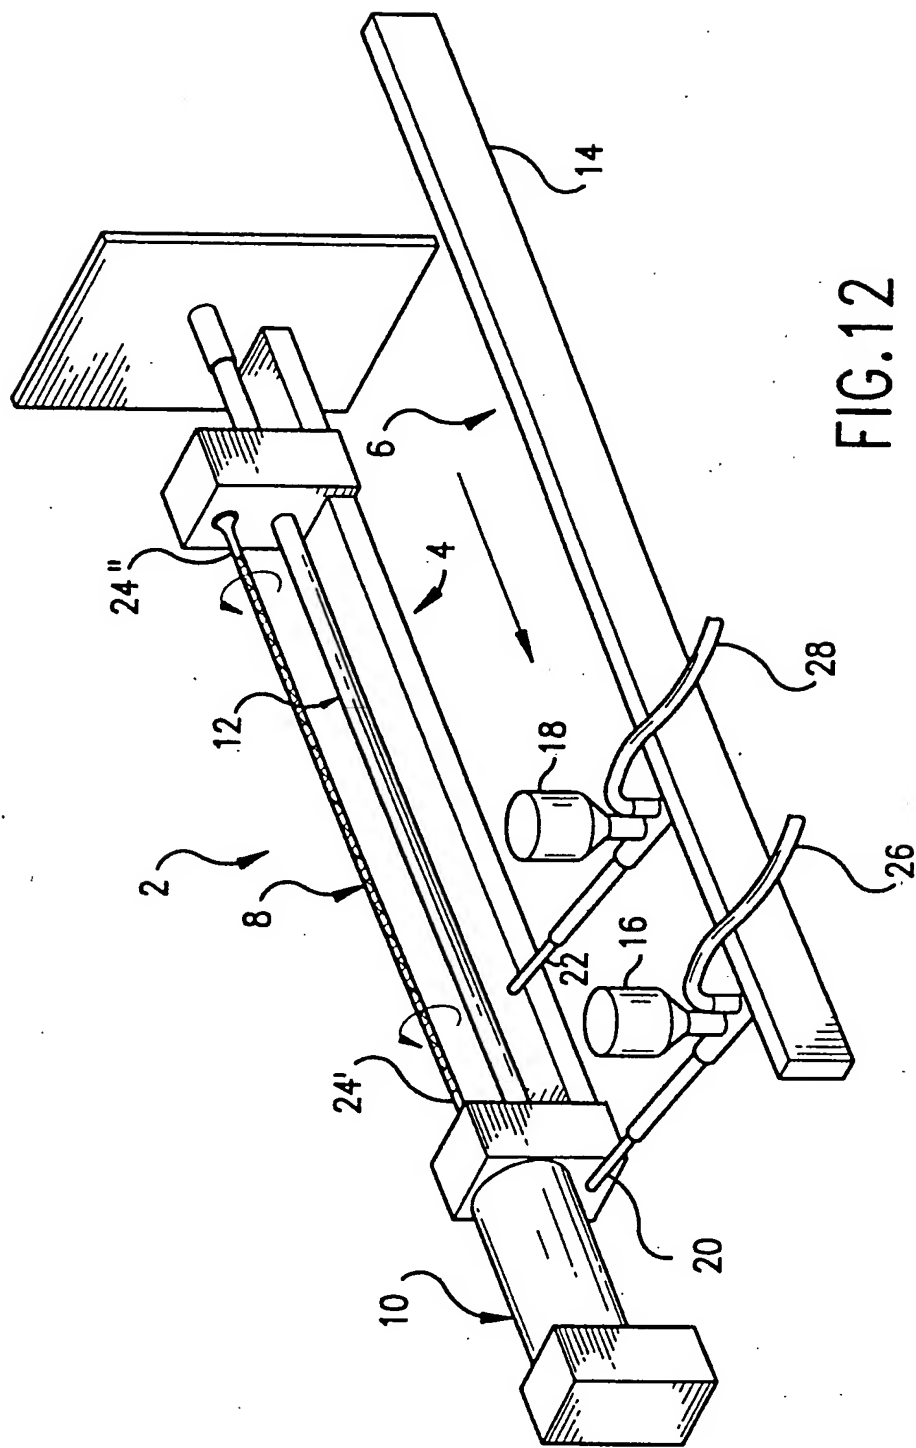


FIG.12



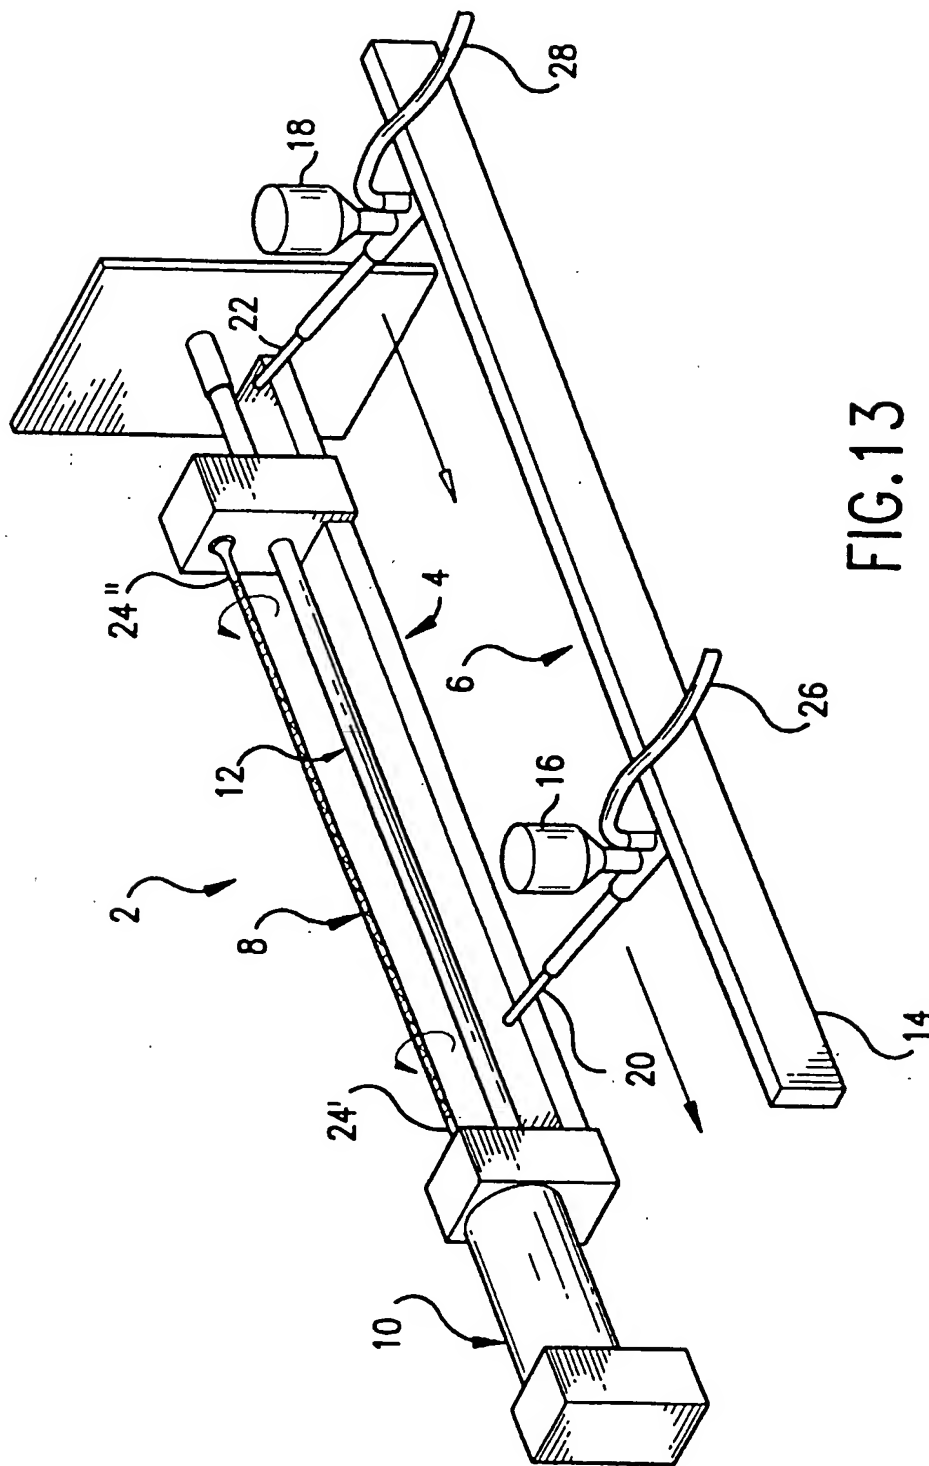


FIG. 13

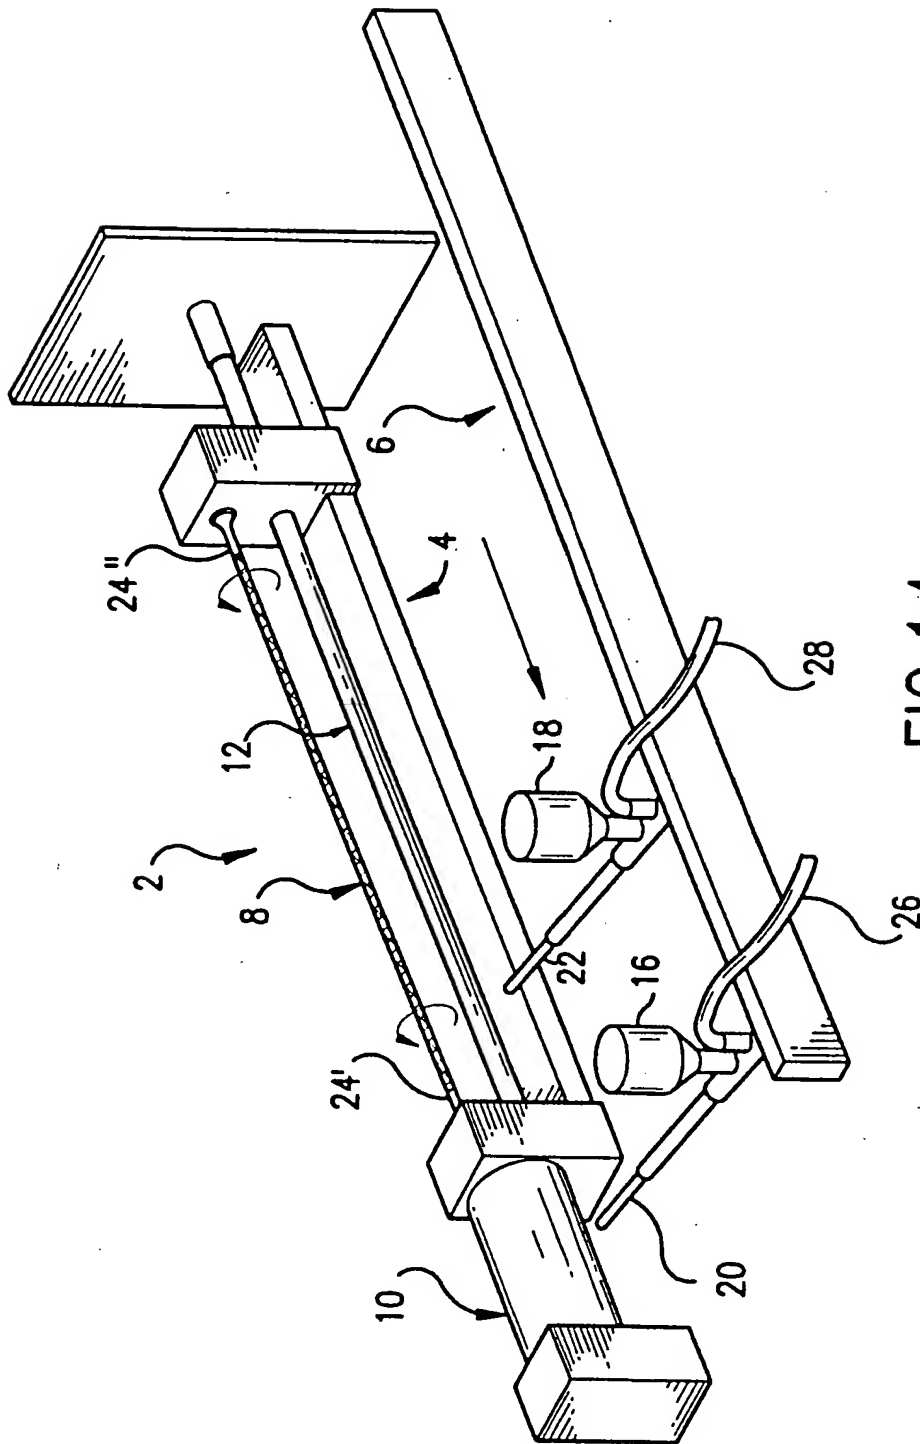


FIG. 14

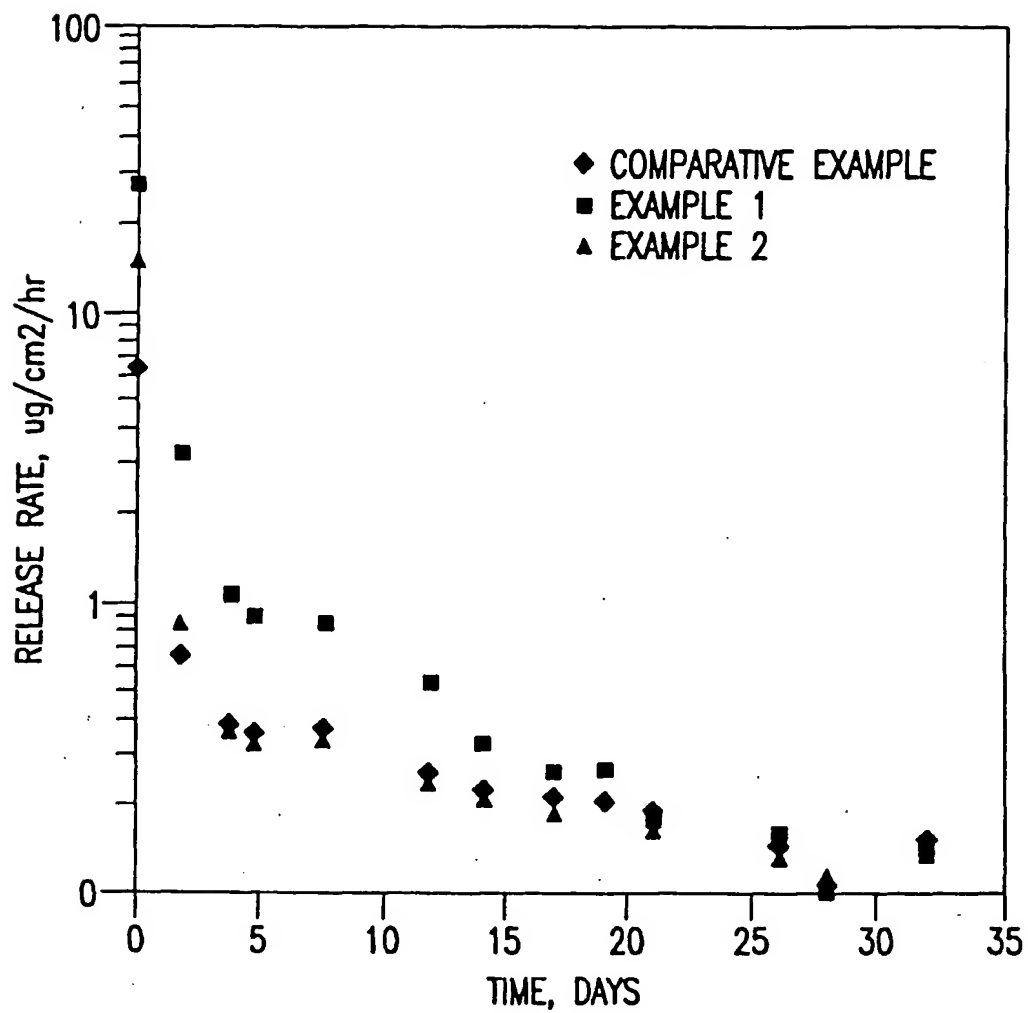


FIG.15


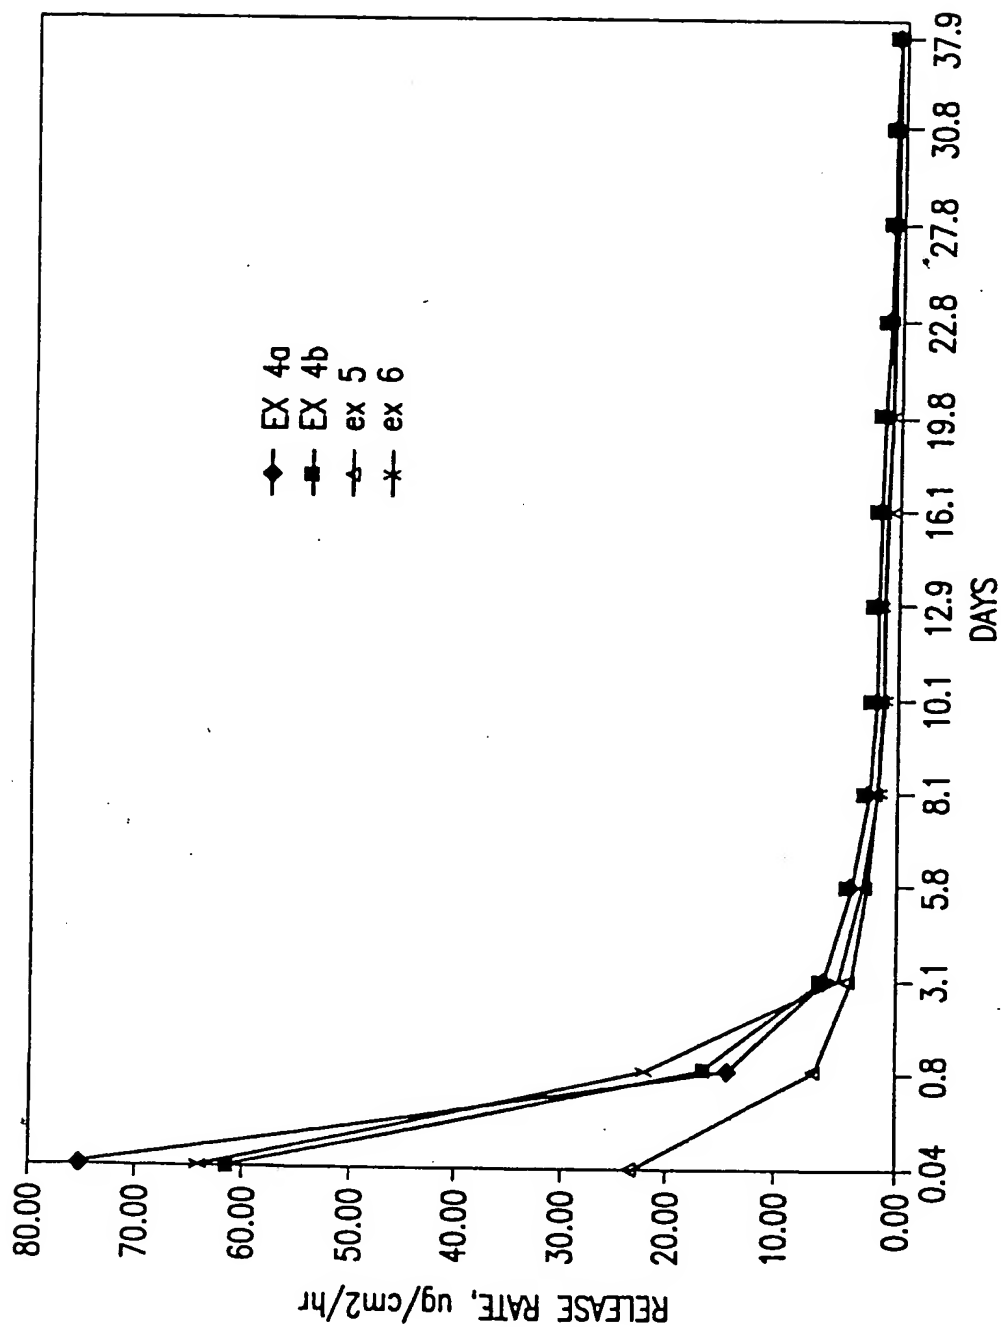


FIG.16



Europäisches Patentamt  
European Patent Office  
Office européen des brevets

(11) EP 0 850 651 A3

(12) EUROPEAN PATENT APPLICATION

(88) Date of publication A3:  
16.08.2000 Bulletin 2000/33

(51) Int. Cl.<sup>7</sup>: A61L 27/00, A61L 31/00

(43) Date of publication A2:  
01.07.1998 Bulletin 1998/27

(21) Application number: 97203933.3

(22) Date of filing: 15.12.1997

(84) Designated Contracting States:  
AT BE CH DE DK ES FI FR GB GR IE IT LI LU MC  
NL PT SE  
Designated Extension States:  
AL LT LV MK RO SI

(30) Priority: 20.12.1996 US 33443 P

(71) Applicant: SCHNEIDER (USA) INC.  
Plymouth, Minnesota 55442 (US)

(72) Inventor: Ding, Ni  
Plymouth, Minnesota 55446 (US)

(74) Representative:  
Gaunt, Robert John et al  
Stevens, Hewlett & Perkins  
Halton House  
20/23 Holborn  
London EC1N 2JD (GB)

(54) Method of applying drug-release coatings

(57) The invention is directed to a method of applying drug-release coatings whereby a polymer can be dissolved in a first solvent (solvent A) to form a polymer system and a drug can be dissolved or suspended in a second solvent (solvent B) to form a drug system. The coating or layer of coating so formed comprises a substantially uniform combination of the drug and polymer. Solvent B can be the same as or different than solvent A. The coating can be applied on a stent body by separately spraying or dipping the polymer system and the drug system onto the devices. The coating can be accomplished by either applying the polymer and drug systems sequentially or simultaneously. In certain embodiments, a drug can be suspended in solvent B. In some cases, three or more systems can be utilized. For instance, a third system containing pure solvent A or B can smooth the coating surface, if the solvent of the third spraying system is compatible with the polymer matrix.

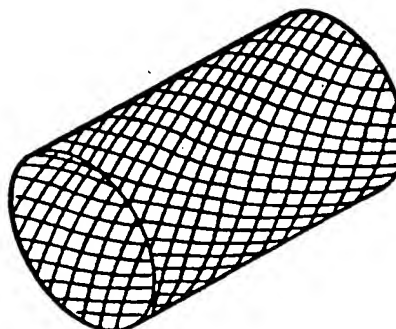


FIG. 10

EP 0 850 651 A3



European Patent  
Office

# EUROPEAN SEARCH REPORT

Application Number  
EP 97 20 3933

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (InCL.6)
X	WO 94 21308 A (CEDARS SINAI MEDICAL CENTER) 29 September 1994 (1994-09-29) * claims; examples 1- *	1-19	A61L27/00 A61L31/00
X	WO 92 15286 A (SHIKANI ALAIN ;NOVA PHARM CORP (US)) 17 September 1992 (1992-09-17) * claims; examples *	1-19	
X	EP 0 623 354 A (MEDTRONIC INC) 9 November 1994 (1994-11-09) * claims; examples 1-7 *	1-10, 12-14	
X	US 5 304 121 A (SAHATJIAN RONALD) 19 April 1994 (1994-04-19) * claims; examples 1,2 *	1-10, 12-14	
X	WO 89 04682 A (COLORADO BIOMEDICAL INC ;BAYSTON ROGER (GB); GROVE NANCY JANE (US)) 1 June 1989 (1989-06-01) * claims *	1,2	
X	US 5 356 433 A (ROWLAND STEPHEN M ET AL) 18 October 1994 (1994-10-18) * examples 1-5 *	1,2	TECHNICAL FIELDS SEARCHED (InCL.6) A61L
X	US 5 053 048 A (PINCHUK LEONARD) 1 October 1991 (1991-10-01) * claims; examples *	1,2	
Y	EP 0 533 262 A (KONTRON INSTR HOLDING) 24 March 1993 (1993-03-24) * claims *	1-25	
Y	WO 91 17724 A (HARBOR MEDICAL DEVICES INC) 28 November 1991 (1991-11-28) * examples *	1-25	
		-/--	
The present search report has been drawn up for all claims			
Place of search THE HAGUE		Date of completion of the search 21 June 2000	Examiner ESPINOSA, M
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

EPO FORM 1503 03 82 (Pct/C01)

EP 0 850 651 A3

European Patent  
Office

## EUROPEAN SEARCH REPORT

Application Number  
EP 97 20 3933

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int.Cl.6)
A	EP 0 675 315 A (MINIMED INC) 4 October 1995 (1995-10-04) * claims; figure 2 * -----	20-25	
			TECHNICAL FIELDS SEARCHED (Int.Cl.6)
The present search report has been drawn up for all claims			
Place of search <b>THE HAGUE</b>		Date of completion of the search <b>21 June 2000</b>	Examiner <b>ESPINOSA, M</b>
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date O : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

EPO FORM 1503 03 02 (P04C01)

EP 0 850 651 A3  
ANNEX TO THE EUROPEAN SEARCH REPORT  
ON EUROPEAN PATENT APPLICATION NO.

EP 97 20 3933

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on  
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

21-06-2000

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 9421308 A	29-09-1994	EP 0689465 A	03-01-1996
		JP 8507715 T	20-08-1996
		US 5562922 A	08-10-1996
		US 5900246 A	04-05-1999
WO 9215286 A	17-09-1992	AU 1579092 A	06-10-1992
		US 5437656 A	01-08-1995
		US 5344411 A	06-09-1994
		US 5512055 A	30-04-1996
		US 5762638 A	09-06-1998
		US 5695458 A	09-12-1997
EP 0623354 A	09-11-1994	US 5464650 A	07-11-1995
		JP 8033718 A	06-02-1996
		US 5837008 A	17-11-1998
		US 5679400 A	21-10-1997
		US 5624411 A	29-04-1997
		US 5776184 A	07-07-1998
US 5304121 A	19-04-1994	US 5824048 A	20-10-1998
		CA 2098984 A	29-06-1992
		DE 69131486 D	02-09-1999
		DE 69131486 T	17-02-2000
		EP 0565604 A	20-10-1993
		EP 0920843 A	09-06-1999
		ES 2137179 T	16-12-1999
		JP 6503984 T	12-05-1994
		WO 9211896 A	23-07-1992
		US 5674192 A	07-10-1997
		US 5954706 A	21-09-1999
		US 5843089 A	01-12-1998
WO 8904682 A	01-06-1989	WO 9211895 A	23-07-1992
		US 4917686 A	17-04-1990
		AT 117563 T	15-02-1995
		AU 635197 B	18-03-1993
		AU 2725888 A	14-06-1989
		BR 8807811 A	09-10-1990
		DE 3852887 D	09-03-1995
		DE 3852887 T	07-09-1995
		EP 0393100 A	24-10-1990
		JP 6040900 B	01-06-1994
US 5356433 A	18-10-1994	NONE	
US 5053048 A	01-10-1991	NONE	

EPO FORM P4439

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82



EP 0 850 651 A3  
ANNEX TO THE EUROPEAN SEARCH REPORT  
ON EUROPEAN PATENT APPLICATION NO.

EP 97 20 3933

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on  
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

21-06-2000

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
EP 0533262 A	24-03-1993	US 5229045 A	20-07-1993
		JP 5192388 A	03-08-1993
		US 5387621 A	07-02-1995
WO 9117724 A	28-11-1991	AU 7998091 A	10-12-1991
		US 5447724 A	05-09-1995
		US 5569463 A	29-10-1996
EP 0675315 A	04-10-1995	US 5456940 A	10-10-1995
		CA 2143771 A	29-09-1995
		DE 69505444 D	26-11-1998
		DE 69505444 T	11-03-1999
		JP 7280177 A	27-10-1995

EPO FORM P4499

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

